Key Message ...

My lab assures accurate and reliable testing processes.

Desired Outcome

Consistently accurate and reliable test processes

- Pre-analytical
- Analytical
- Post analytical

- Ensure the Quality Manual with quality assurance policies and procedures is accessible to and reviewed by all staff
 - Module 10: Why Was the Outdated Version Used?
- Validate new equipment, reagents, and supplies
 - Module 3: Did You Receive What You Ordered?
 - Module 8: Validation of Test Results
- Review discordant rates and determine appropriate action
 - Cross-cutting: Workstation Set-up

- Review occurrence log for patterns/trends and take corrective action
 - Module 2: Safety Incident Role Plays
- Periodically observe/assess accuracy of personnel's work and take corrective action
 - Module 1: Competency Assessment

Bonus Question

• Which section - Key Area of Work – in the Framework has three tasks that refer to SOPs?

Answer


- Section or Key area of Work 6
- Note tasks 6.2, 6.10 &6.11
- Additional related tasks1.4, 1.6, 1.7, 7.3, 8.1,10.1

- 6.2 Ensure the QC material is tested according to SOP
- 6.10 Customize site-specific SOPs as needed
- 6.11 Ensure that SOPs are read and understood by staff

Using Standard Operating Procedures

Standardizing Best Laboratory Practices

Job Aid depicting a Standard Operating Procedures - SOP

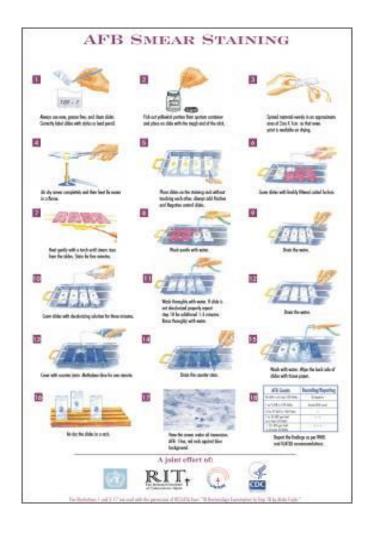

Activity: Using Standard Operating Procedures

Purpose

To write and follow a simple SOP on handwashing

What will you need?

Handout 1: Hand Washing Article

Job Aid 1: SOP Template

Job Aid 2: Annotated SOP

Flipchart pages & markers

What will you do?

- Read <u>Handout 1</u> for OVERNIGHT HOMEWORK
- Use <u>Handout 1</u> and <u>Job Aid 1 & 2</u> as needed to write a simple 7-step SOP on hand washing
- Record the SOP on the flipchart pages
- One group to demonstrate the SOP written by another group
- Participate in the classroom discussion

20 minutes for writing



Demonstration Time

- Let's see if these SOPs are -
 - Complete
 - Easy to follow
 - Yield Accurate & Consistently Reliable Results



Another Bonus Question

- Name one Checklist Item that defines how to use SOPs?
- Checklist Items
 - 1.4, 1.5, 1.6, 1.7, 3.4, 3.7, 5.6, and 8.6

- Establish acceptable ranges for control material
- Track test performance (e.g. Levey-Jennings chart) for trends
- Review records of environmental checks and QC trends to assess impact on testing and take corrective action
- Monitor reagent performance
- Enroll in EQA program, monitor results, and take corrective action

Activity: Is QC That Important

Purpose

To voice and examine the behavior and attitude applied at the worksite regarding quality control.

What will you need?

Worksheet: QC Program Questions

What will you do?

- Complete the <u>Worksheet</u> as homework the evening before this activity
- Participate in the classroom discussion for each question on the <u>Worksheet</u>
- Share your viewpoints openly and respectfully throughout the discussion and listen to others in the same manner.

40 minutes

Knowing where you are and where you want to be starts with creating the right graph.

Is There More to QC Than Just Plotting the Data?

Wrong Patient Results Can:

- Endanger patient lives.
- Prolong suffering.
- •Add significant cost (money and time) to patient treatment.

The right QC approach will detect and prevent errors.

Categories of QC

Quantitative

- Measures the quantity of an analyte
- Numeric
- 5.2 mmol/L

Semi-quantitative

- Measures the quantity of an analyte
- Estimate
- trace, moderate, +1, +3

Qualitative

- Presence or absence
- Positive, negative, growth, no growth, reactive, nonreactive

Statistical QC

- Mean (x̄)
 - the average of a set of values
 - primary indicator of accuracy
 - measure of systematic error (error in a given direction)
- Standard deviation (SD)
 - used to measure dispersion/scattering of a group of values around a mean
 - primary indicator of precision
 - measure of random error (error in any direction)

Mean

$$\overline{\mathbf{X}} = \underline{\sum_{i}}$$

 X_i = individual value

N = number of individual values

Standard Deviation

$$SD = \frac{\sum (x_i - x)^2}{N-1}$$

 $\Sigma = \text{sum (of the differences)}$


 X_i = individual value

X = mean of individual values


N = number of individual values

Confidence Limits

- •Based on normal distribution of results (a bell-shaped frequency curve) a control result will have the following confidence limits:
- •68% will be 1 standard dev. above and below the mean
- •95% will be 2 SD above and below the mean
- •99% will be 3 SD above and below the mean
- •95% confidence limits are the most important limits used.

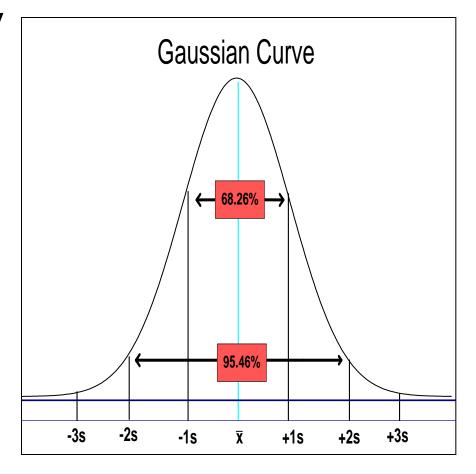

Levey-Jennings Chart

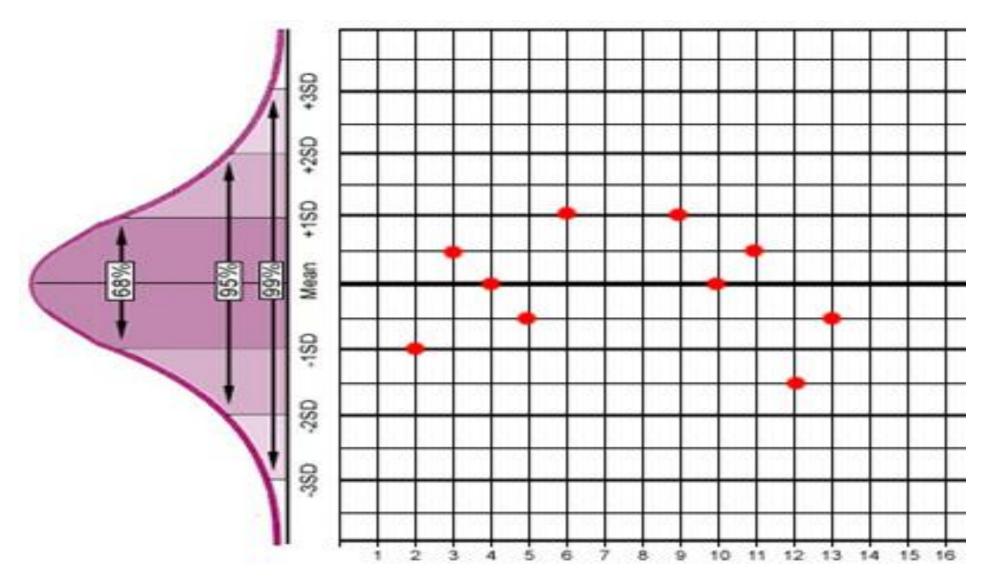

Activity: Is There More to QC than Just Plotting the Data?

Purpose

To demonstrate control range and rule selection's effect on the error detection level of a QC system.

What will you need?

Worksheet 1: Normal Control

Worksheet 2: Data Points

Worksheet 3: L-J Charts

What will you do?

Work individually during the first part of the activity to complete Worksheet 1

For the second half, work with a partner (pairs) to chart data points using Worksheet 1, 2 & 3

- Simple arithmetic used in the worksheets
- Apply different rules and assess level of error detection

The state of the s

25 minutes

Establishing Quality Control Range

Step 1:

 Run new control daily for 20-30 data pts. Run in parallel with current control material

 All new controls must be within the manufacturer's product package insert range

Step 2:

- Calculate from the 20-30 data points of the new control:
 - the mean
 - the standard deviation (1 S.D.)

- From the mean and standard deviation, calculate:
 - +/- 1 S.D.; +/- 2 S.D.; and =/- 3 S.D.

The following information was included in the control's package insert:

Chemistry Normal C	ontrol	Lot # 13427N	Expi	ration Date 15/04/XX
Analyte		Mean (X)		SD
Creatinine		80 umol/L		10 umol/L

You analyzed 30 control samples on your chemistry analyzer, the Illustra 200, and calculated the following values based upon your instrument's control results:

Chemistry Normal C	Lot # 13427N	Expi	ration Date 15/04/XX	
Analyte		Mean (X)		SD
Creatinine		81 umol/L		4 umol/L

Complete the following table using the information above


	Values Using the Package Insert's x and SD	Values Using Your Instrument's x and SD
$\bar{\mathbf{x}}$	80	81
+ 1 SD	90	85
+2 SD	100	89
+3 SD	110	93
- 1 SD	70	77
- 2 SD	60	73
-3 SD	50	69
68% of the data will fall between (± 1SD)	70 - 90	77 - 85
95% of the data will fall between (± 2SD)	60 - 100	73 - 89
99% of the data will fall between (± 3SD)	50 - 110	69 - 93

Cape Clinic Laboratory


L-J Chart for Illustra 200 Chemistry Analyzer

From: <u>May 1, 20XX</u> Through: <u>May 20, 20XX</u>

Use This Graph to Create and Plot the Package Insert Values

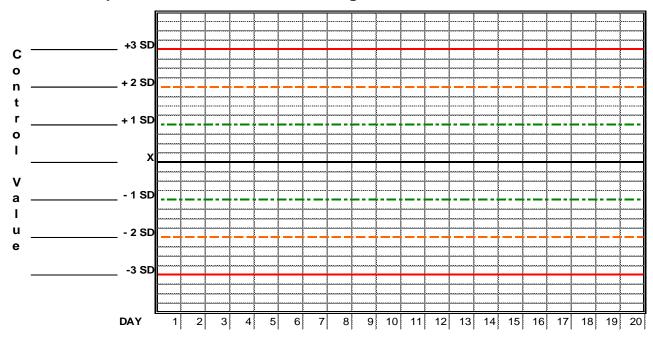

Use This Graph to Create and Plot the Instument's Calculated Values

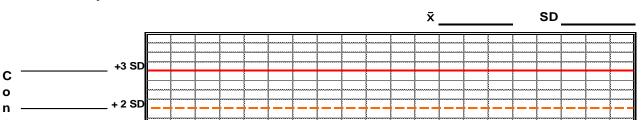


Cape Clinic Laboratory L-J Chart for Illustra 200 Chemistry Analyzer


Analyte: Creatinine Control Material: Normal Units: umol/L

From: <u>May 1, 20XX</u> Through: <u>May 20, 20XX</u>

Package Insert Values

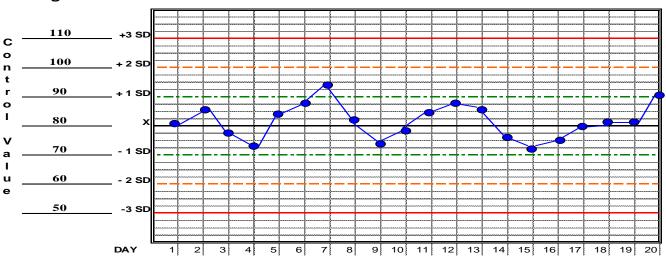

Instument's Calculated Values

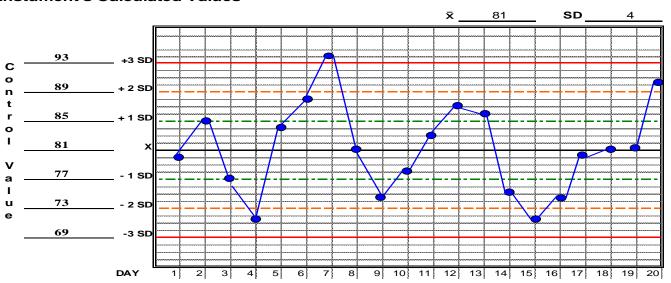

 1_{2s} rule and 1_{3s} rule violations using the instrument's mean and SD chart values.

Day	Normal Control Value	1 _{2s} Violation	1 _{3s} Violation
	0.0	Violation	Violation
1	80		
2	85		
3	77		
4	72		
5	84		
6	88		
7	94	$\sqrt{}$	
8	81		
9	74		
10	78		
11	83		
12	87		
13	86		
14	75		
15	71		
16	74		
17	80		
18	81		
19	81		
20	90	V	

4	1

It makes a difference what control rule(s) is/are applied to accept or reject a run. 4 rejections using the 1_{2s} rule versus 1 rejection using the 1_{3s} rule.

Common QC Terms

- Control Rule a decision criteria to assess whether an analytical run is in-control or outof-control.
 - Single-rule uses a single criterion or a single set of control limits such as 1_{3s or} 1_{2s}.
 - Multirule uses a combination of decision criteria such as 1_{3s}/2_{2s}/R_{4s}.
- Analytical Run the interval (time or a group of samples) for which a decision on acceptability (in-control or out-of-control) is made.

Choice of Quality Control Rules

- Control rules should be carefully selected to maximize error detection and minimize false rejection
- The best set of control rules will vary from method to method and will be based upon:
 - the allowable error required by the test
 - the imprecision and inaccuracy of your method

How QC Works for You

- Calculate the mean and SD of the control material for a single data population.
- Use the calculated mean and SD on the QC chart.
- Use the right QC rules for your method
- Plot the control values versus time on a control chart.
- If a significant change occurs in accuracy or precision, then the QC rule failures alert you to the change.
- Investigate, resolve, and document the rule failure before patient results are reported.

Periodic Review

- Daily review of control values and control charts by the technologist before accepting or rejecting the analytical run.
- Weekly review of QC data and charts by the supervisor
- Monthly review of QC data and charts by the director of the laboratory
- Periodic quality audits by the quality assurance department


Cape Clinic Laboratory

L-J Chart for Illustra 200 Chemistry Analyzer

 Analyte: <u>Creatinine</u>
 Control Material: <u>Normal</u>
 Units: <u>umol/L</u>

 Lot #: 13427N
 Exp Date: 15/04/XX x̄ 81
 SD 4

From: May 1, 20XX Through: May 20, 20XX

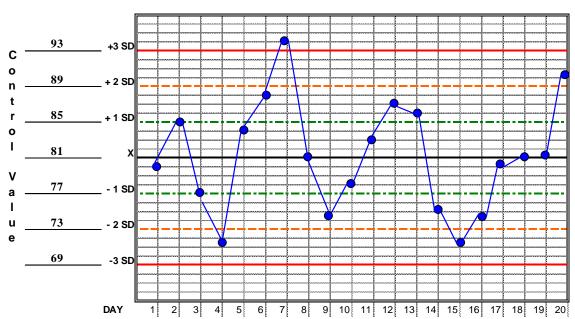

Reviewed 3/5/XX AM Found

Reviewed 20/5/XX AM

- Reviewed 2000/4, with discuss AM

- Por Doy

For En

Reviewed 17/5/XX AM

Reviewed 17/5/XX

Internal and External

- Internal QC- detecting problems during routine laboratory operations.
- External Quality Assessment (EQA)
 - A group of laboratories analyze the same specimens and submit their results to an external facility.
 - Compares your laboratory to a peer group with regard to accuracy and precision of your method.
 - Types of EQA
 - Peer Comparison
 - Proficiency Testing

Activity: Workstation Set-up

Purpose

To create and organize an efficient and productive workstation using elements developed from each module.

What will you need?

Laboratory Accreditation Preparedness Checklist

What will you do?

- Participate in the classroom's discussion
- Integrate key concepts from earlier activities



URINALYSIS DAILY Q.C. LOG AND MAINTENANCE

Multistix	10	SG:	1						Chek-S	stix Combo	Pak:			
lot #:			SG101				Positive Con	ntrol			Negative	Control		
				_				lot#	P83		_	lot#	N83	
exp. date			11/11/XX	-				exp. date	1/15/XX		-	exp. date	1/15/XX	
EXPECT	ED		negative	neg	neg	neg	1.010 - 1.025	6.0 - 7.0	neg	0.2 - 1	neg	neg	neg	
RESULT	S		positive	trace - 250	pos	trace - 80	1.000 - 1.015	8.0 - 9.0	trace- 100	2.0 - 8.0	pos	mod - large	trace-moderate	
	C	C	units	mg/dl		mg/dl			mg/dl	EU/dl				ı
Date	e a n	C a l	Control	Glu	Bili	Ket	S.G.	рН	Prot	Urobili	Nit	Blood	Leuk	Initials
2/03/XX	✓		negative	neg	neg	neg	1.0 20	6.5	neg	0.2	neg	neg	neg	LLC
		✓	positive	250	pos	40	1.0 <i>O</i> 5	8.5	30	8.0	pos	large	mod	
3/03/XX	✓		negative	neg	neg	neg	1.0 20	6.5	neg	0.2	neg	neg	neg	LLC
		~	positive	250	pos	40	1.0 <i>O</i> 5	8.5	30	8.0	роз	mod	mod	
3/03/XX New bottle	ahene	d;	negative	neg	neg	neg	1.0 20	6.5	neg	0.2	neg	neg	neg	LLC
same lot#	7,5		positive	250	pos	80	1.0 15	8.5	30	8.0	pos	large	mod	
			negative				1.0							
			positive				1.0							
			negative				1.0							
			positive				1.0							İ

AFB Stain Log

Manufacturer: Microtrek, In	C
-----------------------------	---

ZN Carbolfuchsin	Decolorizer	Methylene Blue	Results	Initials	Date
12	$I\mathcal{D}$	IM	15 - A	LLC	7/8/XX
12	$I\mathcal{D}$	1M	25 - A	LLC	7/8/XX
1 Z	1 D	1 M	1S - A	AT	9/8/XX
1 Z	1 D	1 M	2S- A	AT	9/8/XX
12	2D	1M	15 - A	LLC	13/8/XX
12	2D	1M	25 - A	LLC	13/8/XX

			Expiration			Expiration	
Reagent	Reagent Code	Lot Number	Date	Code	Lot Number	Date	
TB Ziehl Neelsen							
Carbolfuchsin	1Z	C837	2/11/XX	2Z			
TB Decolorizer (3%							
acid alchohol)	1D	D837	2/11/XX	2D	D954	15/12/XX	
TB Methylene Blue	1M	<i>B837</i>	2/11/XX	2M			
	QC Slide						
Manufacturer	Reagent Code	Lot Nu	mber		Expiration Da	te	
Manufacturer <i>Microtrek</i>	Reagent Code	Lot Nu	mber		Expiration Da	te	
	Reagent Code	Lot Nu			Expiration Da	te	
Microtrek	Reagent Code				•	te	
Microtrek Positive (M. gordonae) Microtrek					•	te	
Microtrek Positive (M. gordonae)					•	te	

Positive control expected result: red bacilli Negative control expected result: blue bacilli Interpretation: A = Acceptable control results

F = Control results are Not acceptable

Complete an Occurrence Report Form if results are not acceptable. Comments:

Supervisor Review: Theresa Rhinehardt

Date: 31/08/XX

38

Glucometer QC Maintenance and QC Log

Calibration /Test	Strip:	Control Level	LOW	NORMAL	HIGH
Lot Numbe	r_#654 /# 977	Lot Number	L835	N721	H854
Expiration Date	7/06/XX / 12/12/XX	Expiration Date	2/1/XX	2/1/XX	2/1/XX
Glucometer #2: Outp	atients SN #2875S	Opened Date	10/04/XX	13/04/XX	08/04/XX
Daily: Verify test strip matches with display Run three control levels each day of use & plot		Expected Range (mmol/L)	2.5 - 3.5	4.5-5.5	21.0 - 23.0
With New Lot# of Strips: Change code chip Run three control levels	As Needed: Change Battery Clean Glucometer with a damp cloth	Opened Expiration Date of Vial (90 days)	9/07/XX	12/07/XX	07/07/XX

Date	Display Lot # matches Test Strip Lot #?	Control Level	Control Result (mg/dl)	QC Plotted	Initials
		Low	2.7	✓	
		Normal	4.9	✓	
30/05/XX	✓	High	22.1	✓	RSM
		Low	3.0	✓	
	_ [Normal	5.0	✓	
3/06/XX	✓	High	22.4	✓	ABL
		Low	2.8	✓	
		Normal	4.6	✓	
5/06/XX	✓	High	21.7	✓	RSM
		Low			
		Normal			
		High			
		Low			
		Normal			
	000000	High		77707774	

Action Item			
New batteries installed, notified supervisor - one set of			
batteries available	RSM		
New Lot number of test strips in use; code chip inserted	RSM		
	New batteries installed, notified supervisor - one set of batteries available		

Reviewed by / date:

AM 3/6/XX

AM 11/6/XX

Initials:

u HCG QUALITY CONTROL LOG

		Kit		QC				
	Kit Lot	Expiration	QC Lot	Expiration			Control Line	
Date	Number	Date	Number	Date	Control	Results	Present	Initials
11/06/XX	SA 721	15/12/XX	SA 721 N	15/12/XX 15/12/XX	negative	+ /_	Y / N	LLC
11/00/11/1	3A 721	15/12/101	SA 721 P	15/12/XX	positive	+ / -	(Y)/ N	
12/06/XX	SA 721	15/12/XX	SA 721 N	15/12/XX	negative	+ / •	Y / N	TII
			SA 721 P	15/12/XX	positive	/ -	Y/N	79
					negative	+ / -	Y / N	
					positive	+ / -	Y / N	

Corrective Action:
Date:

RESULT LOG BOOK (example)

		Control Line			
Date	Patient Name	uHCG	Present	Initials	
11/06/XX	Ramos, Lucínda	positive	✓	LLC	
	Martek, Elizabeth	negatíve	✓	LLC	
	Caspella, Janíce	negatíve	✓	LLC	
12/06/XX	King, Mary	negative	✓	14	

Excerpts from Workstation's SOP

Quality Control:

Built-in Control

The appearance of a control line in the "C" region must appear on the membrane for a test to be valid and for a result to be reported. Document the control line result on the

If the colored line fails to appear in the "C" region, then

Qualitative Quality Control:

A positive and negative quality control material must be performed and recorded in the 'uHCG Quality Control Log' for the following instances:

A. each day

B. when opening a new

If either the positive or negative Q.C. is unacceptable, then

Activity: What Would You Do?

Purpose

To integrate the module's lessons and apply them to the case scenario.

What will you need?

Handout: Case Study Scenarios

What will you do?

Divide into groups of 4-5

- Select a spokesperson for your group
- Formulate specific action steps to address the scenario from the Handout.
- The group's spokesperson presents the proposed steps during the 2 minute class report.



42

What Would You Do?

You notice that only one staff member performs testing on EQA (External Quality Assurance) samples. In fact, the EQA survey was not performed last week because that staff member was on holiday. When you questioned the other staff members they explained they are uncomfortable performing EQA tests. During the same discussion, you discover that the staff member who usually performs the tests has been running the samples 5 times to make certain he has the correct result. You know patients' samples are not to be handled in this manner, and it does not reflect your testing process.

How should you handle EQA surveys at your facility?

- Ensure the Quality Manual with quality assurance policies and procedures is accessible to and reviewed by all staff
- Validate new equipment, reagents, and supplies
- Review discordant rates and determine appropriate action
- Review occurrence log for patterns/trends and take corrective action

- Periodically observe/assess accuracy of personnel's work and take corrective action
- Ensure the QC material is tested according to SOP
- Customize site-specific SOPs as needed
- Ensure that SOPs are read and understood by staff

- Establish acceptable ranges for control material
- Track test performance (e.g. Levey-Jennings chart) for trends
- Review records of environmental checks and QC trends to assess impact on testing and take corrective action
- Monitor reagent performance
- Enroll in EQA program, monitor results, and take corrective action